



## CALIBRATION CERTIFICATE

This is to certify that Prana Air "Air Quality Monitor" has been calibrated by us. Details of reference/ Master instruments are given below.

### Particulate Matter:

The calibration of PM10, PM2.5, and PM1 is performed with a TSI make DustTrak II Aerosol Monitor 8530.

### Reference / Master Instrument

Instrument	Make	Serial No.
TSI Dusttrak 8530	TSI Inc. USA	8530 185004

### Calibration Data

#### Environmental Conditions During Calibration

Temperature: 26 °C


Relative Humidity: 55%

Final Correlation

**91%**

R<sup>2</sup> Value

**0.905**

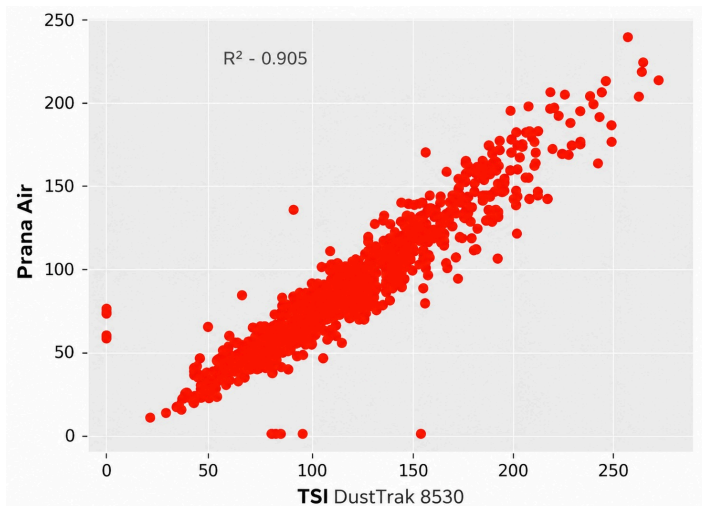

The date of the calibration was on **14/10/2025** (DD/MM/YYYY).

For the next calibration please contact us at **73918-73918**.

Tested: OK

Authorized Signatory

**For PRANA AIR PVT. LTD.**

*Pran Kumar*  
**Auth. Signatory**

**Prana Air Private Limited**



Crown Heights, 7th Floor, 706, Sector-10  
Rohini, New Delhi - 110085, Delhi, India



+91 73918-73918



[www.pranair.com](http://www.pranair.com)